


BUCKINGHAM MFG.

BIG BUCK WRAP PAD

MODEL NO. 3202C & 32021C series - Angled Style Wrap Pad
3204C & 32041C series - Straight Style Wrap Pad.


(Angled Style Wrap Pad shown throughout these instructions)

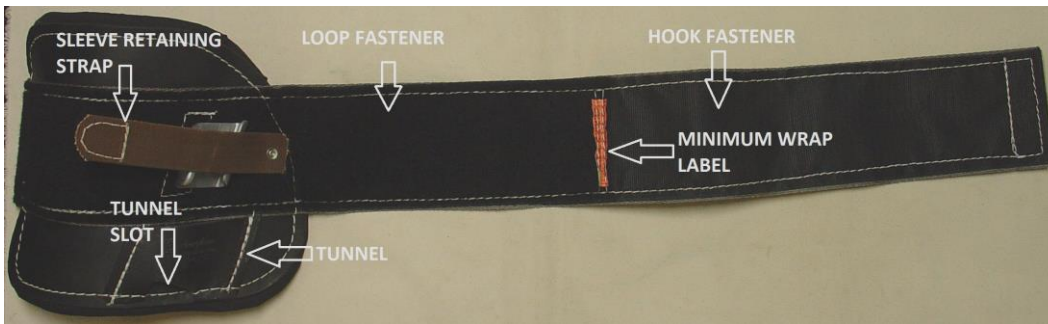

(Right Side shown)

Assembling Pad to Climber

1. Squeeze the pad so the tunnel protrudes outward, away from the pad.
2. Properly orientate climber and push the sleeve (attached to climber) from the bottom upward until the sleeve loop is exposed in the tunnel slot.
3. Adjust the length of the climber using the adjustable climber sleeve so that the top of pad is 1/2" below the projecting knee bone. (Fig. 'A')
4. Slide the sleeve retaining strap under the climber sleeve loop and metal insert loop and pull sleeve retaining strap through both loops.
5. Adhere the sleeve retaining strap to the loop fastener on the pad.

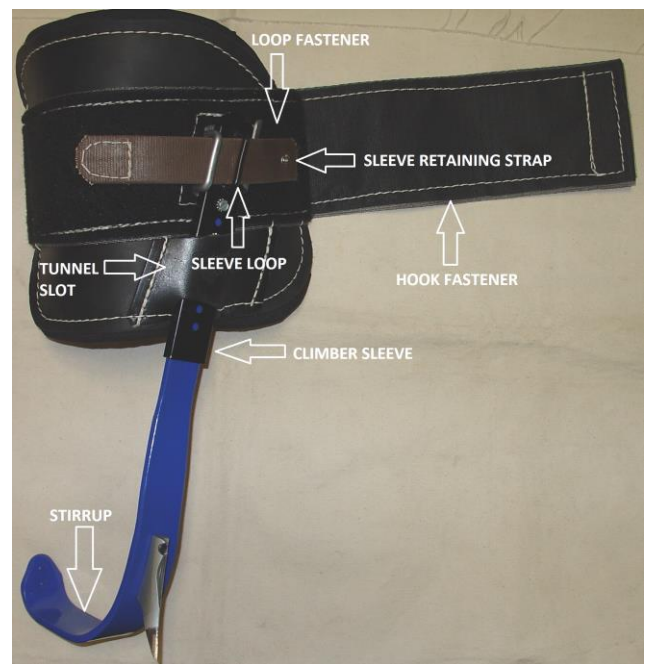

Attaching Pad to Leg

1. Place your foot on the stirrup of the climber with padded fabric portion facing toward the inside of your leg.
2. To secure the pad to your leg, begin by threading the hook and loop strap through the steel loop. (Fig. 'B' and Fig. 'C')
3. Continue to pull the hook and loop strap through the steel loop until the pad is snug on the leg. *Always* ensure that the MINIMUM WRAP LABEL has been pulled through the steel loop. This ensures a proper wrap. Failure to do so may cause release, resulting in serious injury or death. (Fig. 'C' and Fig. 'D')



Fig. 'A'



Fig. 'B'



Fig. 'C'

4. Wrap the free end around the pad, adhering the hook fastener to the loop fastener on the body of the pad. (Fig. 'D')

*Note: Attach and fasten foot strap for climber after attaching pad to leg. (Fig 'A' and 'E')

Cleaning

Proper maintenance and storage of your equipment will prolong its useful life and contribute toward its performance.

Nylon should be cleaned with mild soap and water and be allowed to air dry thoroughly without using excessive heat. Do not use any type of corrosive substance or acid, which will gradually eat away the fabric.

Clean hook & loop fasteners with a soft bristle brush.

Clean leather by removing surface dirt with a clean cloth dampened (not wet) with water and allow to air dry.



Fig. 'D'



Fig. 'E'

STATEMENT of OBSOLESCENCE:

Precise “useful life expectancy” or “shelf life” for this product is not specified, as the degree of use, conditions of use, and the degree of care and storage determines useful life. All users maintain responsibility to select proper equipment for the job, be properly trained in its use, and ensure all personnel support equipment passes inspection before each use. Upon evidence of defects, damage or deterioration, all equipment shall be removed from service immediately and tagged or marked as unusable or destroyed. Additionally, all equipment shall be inspected on a regular basis not to exceed one year by a Competent Person, as defined by OSHA/ANSI, to verify that the equipment is safe for use. In the event of any question or concern regarding the condition of such equipment, users shall remove the equipment from service for further inspection. All users must comply with OSHA/ANSI/ASTM standards prior to and in using such equipment. For more information regarding safe and appropriate use of equipment, please contact Buckingham Manufacturing at 1-800-937-2825.

INTERNATIONAL USERS:

Notwithstanding the above, please know that certain international jurisdictions require manufacturers of equipment to provide customers with a maximum useful lifespan (sometimes referred to as a “Statement of Obsolescence”). To the extent required, Buckingham personal protective equipment manufactured from synthetic fiber materials including but not limited to items such as webbing and/or rope are subject to a maximum useful lifespan of ten (10) years from the date of manufacture. As stated above proper usage, storage, maintenance, and care impacts the useful lifespan of equipment. Extreme circumstances may require that product must be retired after only one use. This statement is made in conformance and compliance with BS EN 365:2004. International users must ensure that product inspections are completed by Competent Persons as defined by international standards including but not limited to British Standard (“BS”). If equipment fails any inspections, it must be immediately withdrawn from service and destroyed. For more information regarding safe and appropriate use of equipment, please contact Buckingham Manufacturing at 1-800-937-2825.

OUR GUARANTEE:

We guarantee the equipment we manufacture to be free from defects in material and workmanship. We will repair any equipment deemed to be defective which is returned to us by the original purchaser. However, this guarantee is void if any product is changed or altered in any way, or if the product is used in a manner other than for which it is intended. This express guarantee supersedes all other expressed or implied guarantees, obligations or liabilities. THERE ARE NO IMPLIED WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE AND AS SUCH, ALL IMPLIED WARRANTIES ARE SPECIFICALLY DISCLAIMED.

LIMITATION ON LIABILITY:

IN NO EVENT WILL BUCKINGHAM OR BUYER BE LIABLE TO THE OTHER FOR LOST REVENUES, LOST PROFITS OR ANY OTHER INDIRECT, CONSEQUENTIAL, SPECIAL OR PUNITIVE LOSSES OR DAMAGES, HOWEVER CAUSED, WHETHER IN ACTION FOR BREACH OF CONTRACT, STRICT LIABILITY, TORT, OR OTHERWISE, EVEN IF ADVISED OF THE POSSIBILITY OF SUCH LOSSES OR DAMAGES. IN NO EVENT WILL BUCKINGHAM'S LIABILITY EXCEED THE TOTAL AMOUNT PAID BY BUYER TO BUCKINGHAM FOR THE PRODUCT OR EQUIPMENT GIVING RISE TO SUCH CLAIM(S).

PLEASE SEE OTHER TERMS AND CONDITIONS RELATING TO THIS PRODUCT AT <https://buckinghammfg.com/terms-conditions/>

REGISTRATION:

Before use of the product, ensure to register and confirm the product at www.buckinghammfg.com/register.

BUCKINGHAM MFG.
BINGHAMTON, NY
1-800-937-2825
e-mail - sales@buckinghammfg.com

Information contained in these written instructions supersedes all other information (written, audio, video etc. produced by Buckingham Mfg. prior to the revision date of this document.